# NATIONAL BUREAU OF STANDARDS REPORT

6433

Progress Report

on

MECHANICAL EVALUATION OF SOME

HIGH SPEED HANDPIECES

by

Duane F. Taylor
Robert R. Perkins
John W. Kumpula

U. S. DEPARTMENT OF COMMERCE
NATIONAL BUREAU OF STANDARDS

## THE NATIONAL BUREAU OF STANDARDS

### Functions and Activities

The functions of the National Bureau of Standards are set forth in the Act of Congress, March 3, 1901, as amended by Congress in Public Law 619, 1950. These include the development and maintenance of the national standards of measurement and the provision of means and methods for making measurements consistent with these standards; the determination of physical constants and properties of materials; the development of methods and instruments for testing materials, devices, and structures; advisory services to Government Agencies on scientific and technical problems; invention and development of devices to serve special needs of the Government; and the development of standard practices, codes, and specifications. The work includes basic and applied research, development, engineering, instrumentation, testing, evaluation, calibration services, and various consultation and information services. A major portion of the Bureau's work is performed for other Government Agencies, particularly the Department of Defense and the Atomic Energy Commission. The scope of activities is suggested by the listing of divisions and sections on the inside of the back cover.

### Reports and Publications

The results of the Bureau's work take the form of either actual equipment and devices or published papers and reports. Reports are issued to the sponsoring agency of a particular project or program. Published papers appear either in the Bureau's own series of publications or in the journals of professional and scientific societies. The Bureau itself publishes three monthly periodicals, available from the Government Printing Office: The Journal of Research, which presents complete papers reporting technical investigations; the Technical News Bulletin, which presents summary and preliminary reports on work in progress; and Basic Radio Propagation Predictions, which provides data for determining the best frequencies to use for radio communications throughout the world. There are also five series of nonperiodical publications: The Applied Mathematics Series, Circulars, Handbooks, Building Materials and Structures Reports, and Miscellaneous Publications.

Information on the Bureau's publications can be found in NBS Circular 460, Publications of the National Bureau of Standards ($1.25) and its Supplement ($0.75), available from the Superintendent of Documents, Government Printing Office, Washington 25, D. C.

Inquiries regarding the Bureau's reports should be addressed to the Office of Technical Information, National Bureau of Standards, Washington 25, D. C.

# NATIONAL BUREAU OF STANDARDS REPORT

| NBS PROJECT | | NBS REPORT |
|---|---|---|
| 0708-20-3824 | June 12, 1959 | 6433 |

Progress Report

on

## MECHANICAL EVALUATION OF SOME HIGH SPEED HANDPIECES

by

Duane F. Taylor*
Robert R. Perkins**
John W. Kumpula'

* Metallurgist, Dental Research Section, National Bureau of Standards.
** Guest Worker, U. S. Navy, Dental Research Section, National Bureau of Standards.
' Laboratory Mechanic, Dental Research Section, National Bureau of Standards.

This work is a part of the dental research program conducted at the National Bureau of Standards in cooperation with the Council on Dental Research of the American Dental Association, the Army Dental Corps, the Dental Sciences Division of the School of Aviation Medicine, USAF, the Navy Dental Corps, and the Veterans Administration.

IMPORTANT NOTICE

NATIONAL BUREAU OF STAI
intended for use within the G
to additional evaluation and re
listing of this Report, either in
the Office of the Director, Nati
however, by the Government a
to reproduce additional copies

Approved for public release by the director of the National Institute of Standards and Technology (NIST) on October 9, 2015

gress accounting documents
ally published it is subjected
production, or open-literature
n is obtained in writing from
uch permission is not needed,
epared if that agency wishes

NBS

U. S. DEPARTMENT OF COMMERCE

NATIONAL BUREAU OF STANDARDS

# MECHANICAL EVALUATION OF SOME HIGH SPEED HANDPIECES


## Abstract

The power transmission characteristics of a series of dental air turbine handpieces were studied. The torque produced as a function of speed was determined for each handpiece tested. The effects of air pressure, instrument size, and instrument balance upon the speed and power were investigated. Increased pressure was found to be more effective in increasing power than in increasing speed. The size of the instrument was found to have negligible effect upon the power output in comparison to the effect of dynamic balance.

# I. INTRODUCTION

The introduction in the last few years of a wide variety of high-speed dental handpieces and instruments has emphasized the need for some method of evaluating dental cutting procedures. The dental literature has been filled with papers related to the use of high speeds, and a complete bibliography on the subject would run to several hundred items for the last five years alone. Only a very few of these papers, however, have been concerned with the mechanism of cutting or the instruments themselves [1-3]. The majority have been directed toward techniques for their clinical use.

The Dental Research Section of the National Bureau of Standards has for several years conducted a program of research into various non-clinical aspects of the dental cutting problem [4-9]. One portion of this program has been the investigation of the mechanical operating characteristics of dental handpieces. This paper presents our findings and conclusions in regard to one group of these handpieces, the air turbines.

The program as a whole is directed toward providing a more fundamental understanding of the cutting process with particular emphasis upon the energy considerations involved. A wide variety of handpieces was studied to

provide basic information in regard to the conditions that are encountered clinically. These handpieces included belt-driven designs having maximum speeds from 6,000 to 150,000 rpm, and water turbines, as well as the air turbines discussed here. It is hoped that this study not only will provide a basis for quantitative measurement of the characteristics of different types of handpieces but also will lead to a better understanding of the cutting process itself.

The method employed involves measurement of the energy transferred at several places within the cutting equipment, most particularly the energy transfer from the handpiece to the instrument and from the instrument to the surface being cut. This permits the comparison of the useful work obtained (cutting) to the losses (heat, noise and vibration) and allows an evaluation of the relative efficiency of various handpiece-instrument combinations. A detailed description of the equipment developed and methods employed in this study appears elsewhere [10], and only a short discussion will be given here.

## II. EXPERIMENTAL PROCEDURE

The air turbines tested are listed in Table 1. As indicated there, the number of samples tested ranged from

one to four. The Midwest handpiece tested was an experimental design employing latch-type burs rather than the friction-grip design presently available. The other handpieces were all standard commercial models.

The operating characteristics of the handpieces were studied by determining the torque delivered to the instrument shaft by the handpiece at various speeds. An overall view of the equipment used for this purpose is shown in Figure 1, while a close-up view with a handpiece mounted for testing appears in Figure 2.

This apparatus was designed to produce a braking effect upon the handpiece by interaction between a synchronous magnetic field and a permanent magnet ferrite cylinder mounted in the handpiece. The braking field was brought into synchronization with the handpiece and the field strength increased until the handpiece speed was controlled by the field frequency. The handpiece speed was then varied by changing the frequency while the torque produced at various speeds was observed.

Calibration and reading errors cause a relative uncertainty of about five percent between the individual observations on a single run for both speed and torque. Absolute values of torque are known to the same accuracy

but drift in calibration of the frequency measuring system induces a maximum additional uncertainty of 5% in the absolute speed determinations.

Results and Discussion

A typical torque-speed relationship found by this technique is shown in Figure 3. The shape of this curve is typical of all of the turbines tested. It has been generally observed clinically that the torque produced by the air turbines is much smaller than that produced by conventional belt-driven handpieces. For example, the maximum torque produced in this run, about 10 gram-centimeters, is attained at minimum speed and may be compared with the 250-300 gram-centimeters maximum torques achieved by typical ball bearing belt-driven handpieces as shown in Figure 4.

The results obtained, particularly in some of the early runs, were not always as regular as those of Figure 3. Data of the type shown in Figure 5 were often obtained and in some cases the curves were as irregular as that shown in Figure 6. In this case, at the air pressure used, (30 psi), the handpiece would reach a maximum speed of only 110,000 rpm. When that speed was approached the handpiece became increasingly noisy and the cylinder ran

very eccentrically. Gradually increasing the air pressure made little difference in the speed until near 50 psi, when the speed suddenly increased to 400,000 rpm. Reducing the pressure to 30 psi produced a free running speed of 360,000 rpm. From that point the torque-speed curve could be traced to 300,000 rpm where the torque dropped toward zero. It was impossible to follow the curve continuously through this range and the middle section (between 300,000 and 100,000 rpm) was derived only by pressure cycling. When this was done, however, it was possible to follow this portion of the curve satisfactorily at 30 psi pressure.

This behavior was attributed to a resonance effect. The regular spacing of the speeds at which reduced torques appear, support this conclusion. Major drops occurred near 100,000 and 300,000 rpm and a smaller drop at 200,000 rpm. Although the magnet cylinders and the handpiece rotors were themselves well balanced, it was conceivable that, when the magnets were inserted in the handpiece, errors of alignment or centering might make the rotor-cylinder combination dynamically unbalanced. As a result, an attempt was made to grind the magnet cylinder into dynamic balance while driving them with the handpiece.

Figure 7 shows three of the magnet cylinders used. The one on the left has been ground and balanced relative to its shaft, while the others have subsequently been balanced in a handpiece. Of the three, the one on the right ran the fastest in spite of its rough appearance. Improvement, when it occurred, was often dramatic though not readily predictable. Table 2 shows the results of a series of successive grinding passes on three cylinders being balanced for the same handpiece.

The particular rotor with which these data were obtained was very sensitive to defects of balancing, although a previous rotor in the same handpiece had shown a much less marked effect.

Somewhat similar, though less extreme behavior was observed with burs. When several burs of the same size were tested, they were commonly observed to run at different maximum speeds. Also, reducing the pressure to the handpiece to levels of 5 to 10 psi at times produced results with burs which closely resembled those with unbalanced cylinders. In the case of the burs, however, increase of pressure back to the normal operating range or removing and repositioning the bur in the handpiece were sufficient to let the handpiece escape the low speed

resonance and achieve normal free-running speeds. Apparently the same type of effects occur with the cylinders and with burs. However, because of the relatively small mass of the burs the effect becomes apparent only under those circumstances where the torque of the handpiece is already marginal, near maximum speed or at very low pressures. Diamond instruments should be expected to produce similar results intermediate to these two cases.

Table 3 illustrates the importance of this factor in determining handpiece speeds. It compares the maximum speeds attained with three magnet cylinders and four burs at a series of pressures. The cylinders were all balanced by grinding in the handpiece used for the tests, a Weber AT 200. Note that of the three cylinders, No. 1 which was the slowest running of the three still shows signs of resonance problems and is apparently not fully balanced. It shows a one-third increase in speed between 20 and 30 psi from 180,000 to 240,000 rpm, (both multiples of 60,000), and not until the pressure was increased to 60 psi was any further increase in speed obtained. The other cylinders and the burs showed a continual increase in speed with pressure.

Probably the most significant point relative to this table, however, is that, in spite of their large size (approx. .240 x .400 inch) and the irregular surface produced in the balancing operation, cylinders 2 and 3 ran as fast or faster than any of the burs. This indicates that size alone is no detriment for high speed operation and that air drag must play a very minor role in controlling speed. It also appears that an eccentric bur or worn chuck that unbalances the rotor can result in considerable slowing of the handpiece and reduced performance.

Typical torque-speed curves for the various handpieces tested with resonance effects eliminated are shown in Figure 8. All curves are for 30 psi air pressure which is the approximate maximum pressure allowed by the regulators in the S. S. White and Ritter handpieces tested.

Of the six curves shown, numbers 1, 2, and 6 are for handpieces using latch-type contra-angle burs while the other three handpieces use friction-grip burs. The use of the larger shank, latch-type bur results in a larger overall head size for the handpiece and appears to require a greater air supply. Of the three latch-type handpieces tested, only one, the Weber AT 200 is marketed at the present time. It has replaced the Weber model 700.

The Midwest handpiece studied has been replaced by a friction-grip handpiece which was not tested.

In those cases where several samples of a single handpiece design were tested, considerable differences in performance were noted. In addition, smaller changes occurred from day to day and run to run with a single handpiece. These variations together amount to as much as ± 15% from the mean and appear to be due mainly to such causes as irregular lubrication and bearing wear.

While the torque-speed curve provides the basic information in regard to the energy transferred from the handpiece to the bur, in many cases, it is more informative as well as more convenient to work with power-speed data. Since the power of a rotating device is equal to the product of the speed and torque, the power-speed curve is readily derived from the torque-speed measurements. The power curves corresponding to the runs of Figure 8 are shown in Figure 9. For comparison the belt-driven handpiece of Figure 4 develops a maximum power of 25.9 watts at 19,000 rpm.

The effect of variations in pressure upon the performance of one air turbine handpiece is shown in Figures 10 and 11. The values given are for the Weber AT 200,

which is shown here because of the range of pressures usable with this handpiece. A wide pressure range is definitely advantageous for laboratory investigation since it permits the study of a variety of speeds and powers with a single handpiece.

The clinical necessity for very high pressures is doubtful and some makes of handpieces have regulators which permit a maximum pressure of 30 psi.

The curves of Figures 10 and 11 show certain characteristics common to all of the air turbines tested. The effect of increasing air pressure is much greater upon the torque than upon the speed. As seen in Figure 10, doubling the air pressure will approximately double the maximum torque developed but will increase the maximum speed only 16%. The influence of design appears to be much more important than air pressure in determining maximum handpiece speed. However, the pressure used may make a considerable difference in the speed reached during cutting. Figure 10 indicates that if the handpiece is required to supply five gram-centimeters of torque to the instrument during cutting, (a high value for this speed range), the handpiece will run 270,000 rpm at 60 psi, 240,000 rpm at 50 psi, 205,000 rpm at 40 psi, 135,000 rpm

at 30 psi, and will stall completely at 20 psi.

Figure 11 shows that the maximum power available increases rapidly with increased pressure. The speed at which the maximum power occurs is also seen to increase with pressure.

Unfortunately, from the clinical point of view, information is not yet available as to how much power is needed or desirable for operative use. It is now possible to make a start in that direction by making cutting tests using handpieces whose operating characteristics are known. Provided with the data of Figure 11, it is possible, for example, to make a series of cuts at a constant speed with varying powers (shown by the dots in Figure 11) or at constant power with varying speeds (shown by crosses). Study of the cutting performed and heat produced under these conditions should permit the determination of the effect of both factors upon cutting efficiency. Such a program has been undertaken in the expectation that it will eventually lead to a better understanding of the dental cutting process as a whole.

## III. SUMMARY

The operating characteristics of several designs of air turbine handpieces have been investigated. Their ability to transmit energy to the shaft of the cutting instrument was studied by means of an electro-dynamic brake, and was found to be strongly dependent upon the dynamic balance of the instrument and upon the air pressure used. This method provides a means for the comparison of various air turbine handpieces and yields data which can be used as a basis for the study of the mechanism and efficiency of dental cutting procedures.

## Bibliography


1. Peyton, Floyd A., Evaluation of Dental Handpieces for High Speed Operations. J.A.D.A. 50: 383-391, April 1955.

2. Bernier, J. L. and Knapp, M. J., Methods Used in Evaluation of High Speed Dental Instruments and Some Results. Oral Surg., Oral Med. and Oral Path. 12: 234-252, February 1959.

3. Rigas, D. J., Skinner, E. W., Lindenmeyer, R. S., and Lasater, R. L., Design Factors of Dental Burs as Related to Cutting Effectiveness, J. D. Res. 37: 91, February 1958, Abstract.

4. Nelsen, R. J., Pelander, C. E. and Kumpula, J. W., Hydraulic Turbine Contra-angle Handpiece, J.A.D.A., 47: 324, September 1953.

5. Hudson, D. C., and Sweeney, W. T., Temperatures Developed in Rotating Dental Cutting Instruments, J.A.D A. 48: 127, February 1954.

6. Hudson, D. C., Hartley, J. L., Moore, Robert and Sweeney, W. T., Factors Influencing the Cutting Characteristics of Rotating Dental Instruments, J.A.D.A. 50: 377, April 1955.

7. Dental Burs in Action. Film available on loan from the Office of Scientific Publications, National Bureau of Standards, Washington 25, D. C., or the American Dental Association Film Library, 222 East Superior St., Chicago 11, Illinois.

8. Hartley, J. L., Hudson, D. C., Sweeney, W. T., and Richardson, W. P., Cutting Characteristics of Dental Burs. Armed Forces Medical J. 8: 209, February 1957.

9. Hartley, J. L., Hudson, D. C., Sweeney, W. T., and Dickson, George., Methods for the Evaluation of Rotating Diamond-abrasive Dental Instruments., J. A. D. A., 54: 637, May 1957.

10. Perkins, Robert R., Taylor, Duane F., and Kumpula, J. W., Evaluation of Dental Cutting Procedure: Method and Apparatus (in preparation).

Table 1

Air Turbine Handpieces Tested

| Handpiece | | | Number of Samples |
|---|---|---|---|
| Densco | Aero Turbex | | 1 |
| Midwest | Air Drive | | 1 |
| Ritter | Air Rotor | | 2 |
| S.S. White | Air Rotor | | 1 |
| Weber * | Air Turbine | 700 | 4 |
| Weber | Air Turbine | AT 200 | 2 |

Table 2

The Effect of Balancing Upon Maximum Rotational Speed

| | Magnet Cylinder | | |
|---|---|---|---|
| | 1 | 2 | 3 |
| Initial Speed | 80,000 rpm | 50,000 rpm | 70,000 rpm |
| 1st Grinding | 85,000 | 75,000 | 220,000 |
| 2nd Grinding | 85,000 | 280,000 | 50,000 |
| 3rd Grinding | 320,000 | -- | 210,000 |

| | |
|---|---|
| Handpiece | Weber AT-200 Air Turbine |
| Pressure | 30 psi |
| Cylinder | .240 Diam. x .400 length approx. |

Table 3

The Effect of Air Pressure Upon the Rotational Speed of Various Instruments

| Instrument | Air Pressure to the Handpiece | | | | |
|---|---|---|---|---|---|
| | 20 psi | 30 psi | 40 psi | 50 psi | 60 psi |
| Cylinder No. 1 | 180,000rpm | 240,000rpm | 240,000rpm | 240,000rpm | 280,000rpm |
| Cylinder No. 2 | 270,000 | 290,000 | 300,000 | 340,000 | 360,000 |
| Cylinder No. 3 | 250,000 | 275,000 | 280,000 | 300,000 | 320,000 |
| No. 700 Bur | 180,000 | 230,000 | 275,000 | 290,000 | 320,000 |
| No. 6 Bur | 200,000 | 225,000 | 250,000 | 275,000 | 280,000 |
| No. 558 Bur | 180,000 | 200,000 | 225,000 | 240,000 | 250,000 |
| No. 35 Bur | 240,000 | 250,000 | 275,000 | 290,000 | 300,000 |

Cylinder diam. .240 inch length .400

Handpiece Weber AT-200

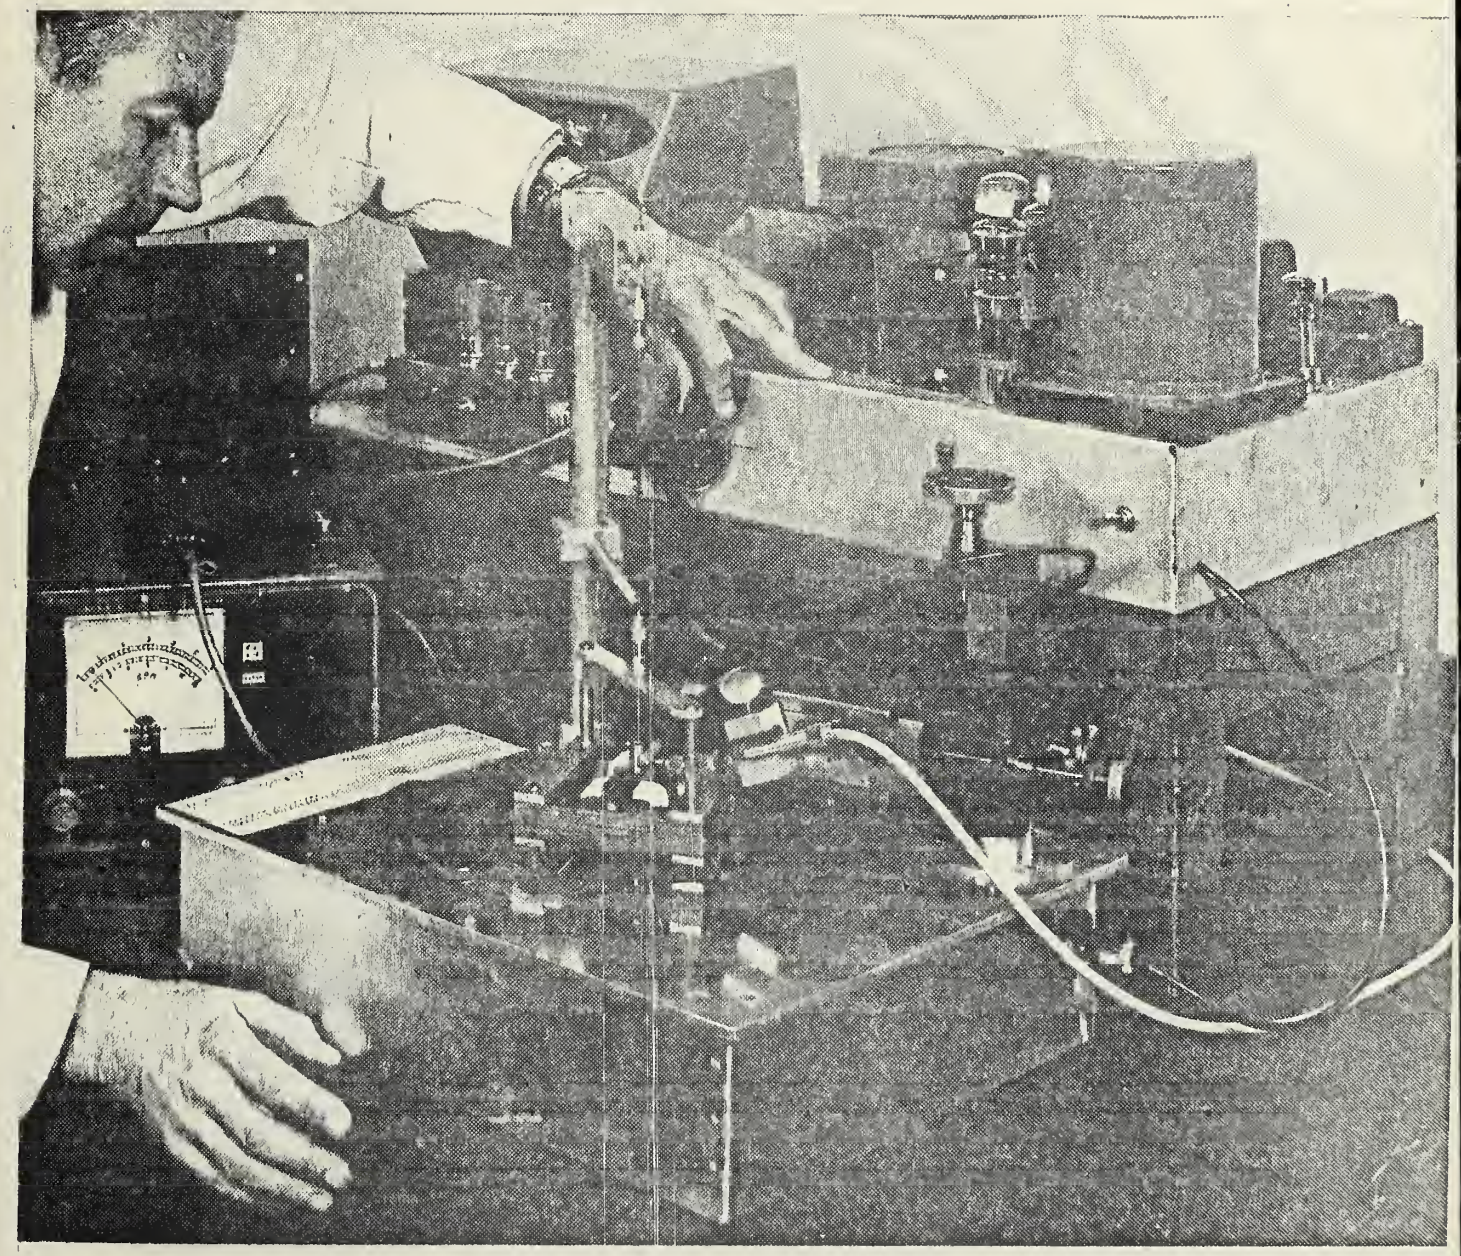

Figure 1. Apparatus employed for the high speed-low torque measurements.



Figure 2. Closeup showing details of the electrodynamic brake.




Figure 3. Torque - speed curve typical of air turbine handpieces.




Figure 4. Torque - speed curve for a typical ball bearing belt driven handpiece.

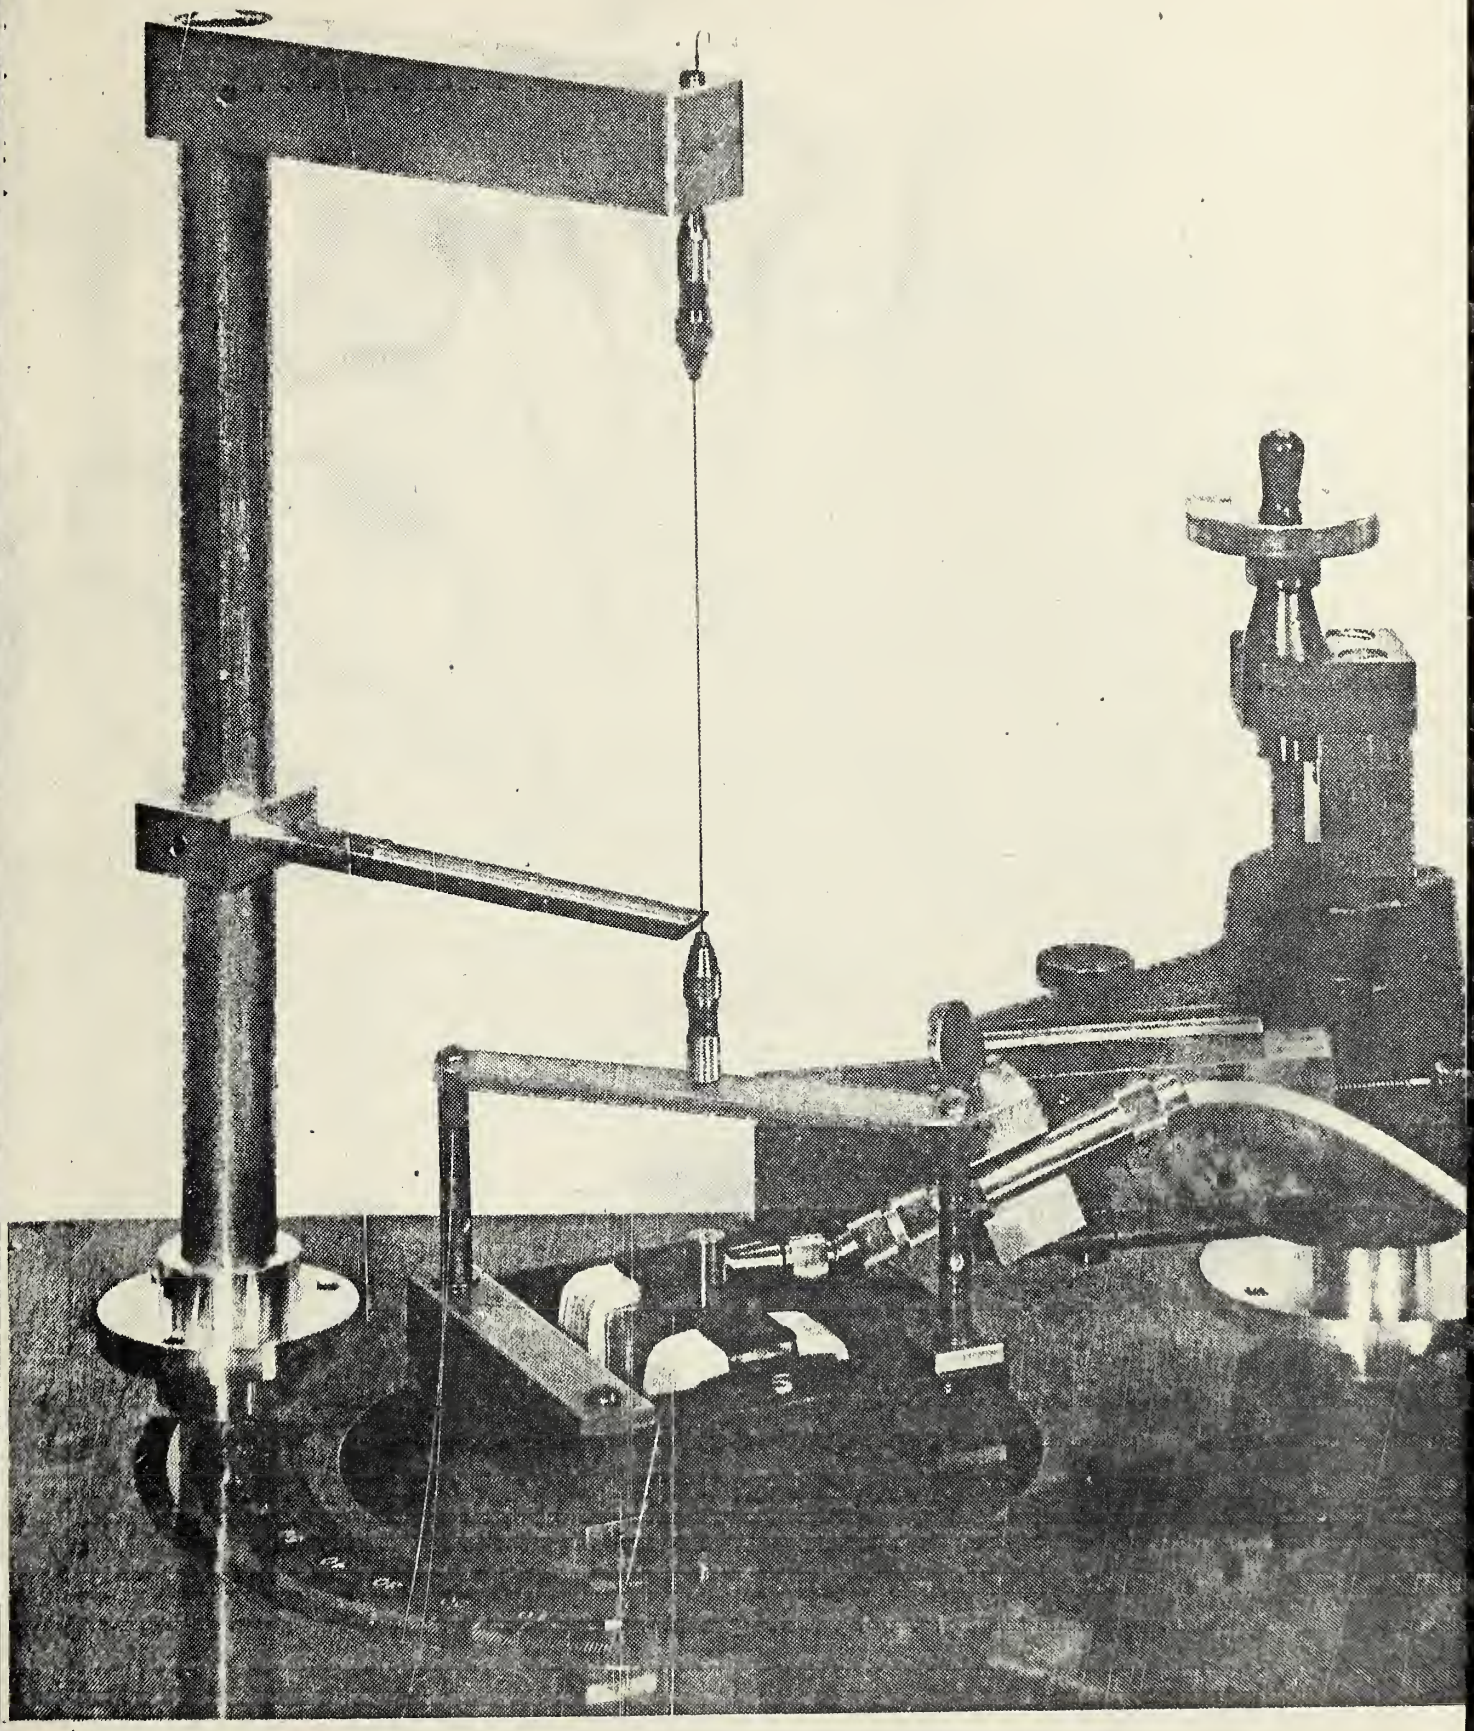


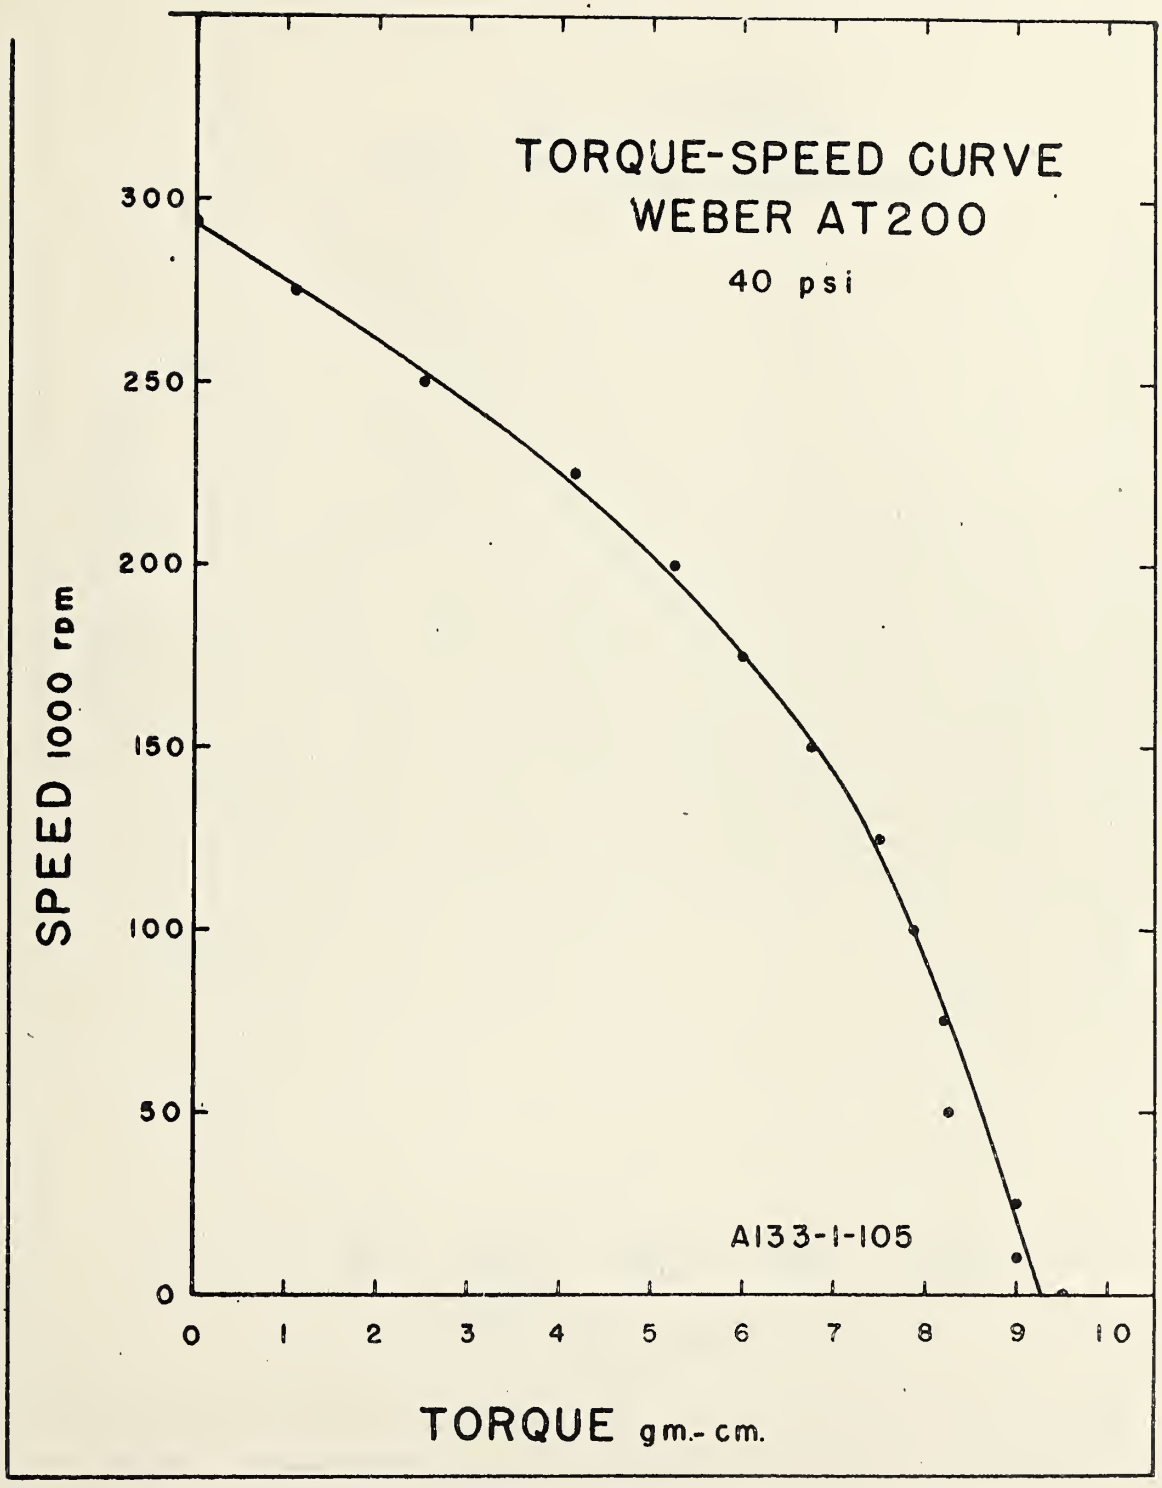Figure 5. Torque - speed curve showing mild resonance effects.

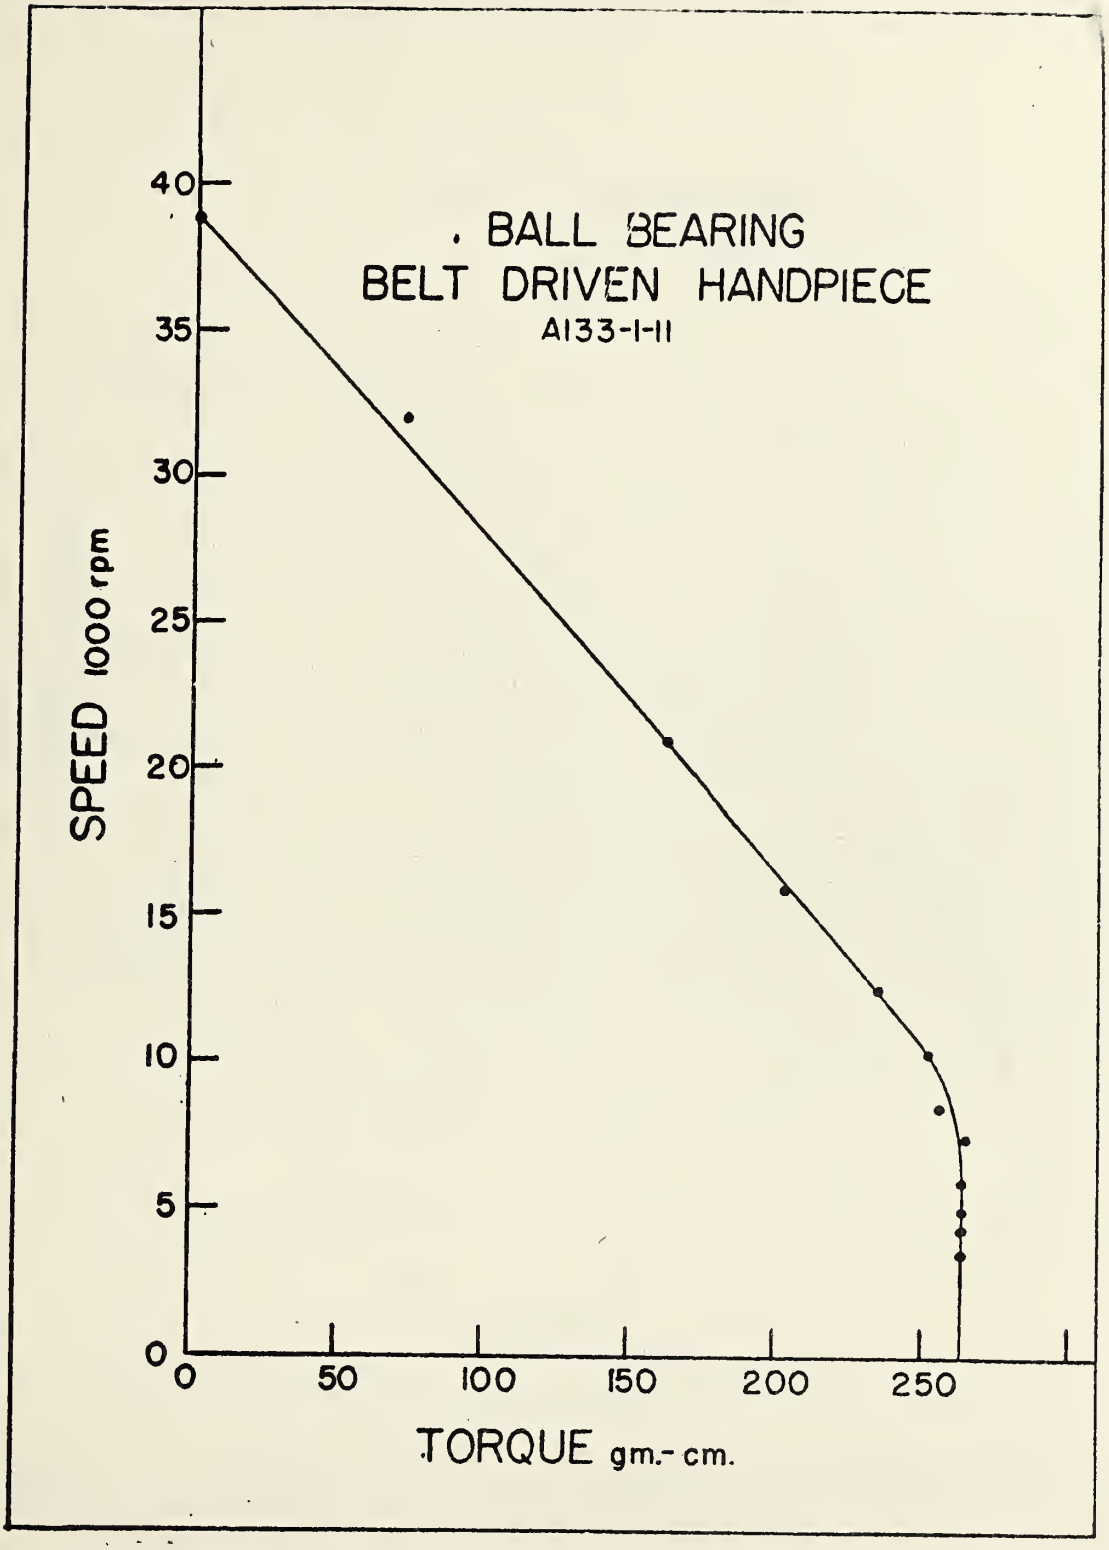


Figure 6. Torque - speed curve showing extreme resonance effects.

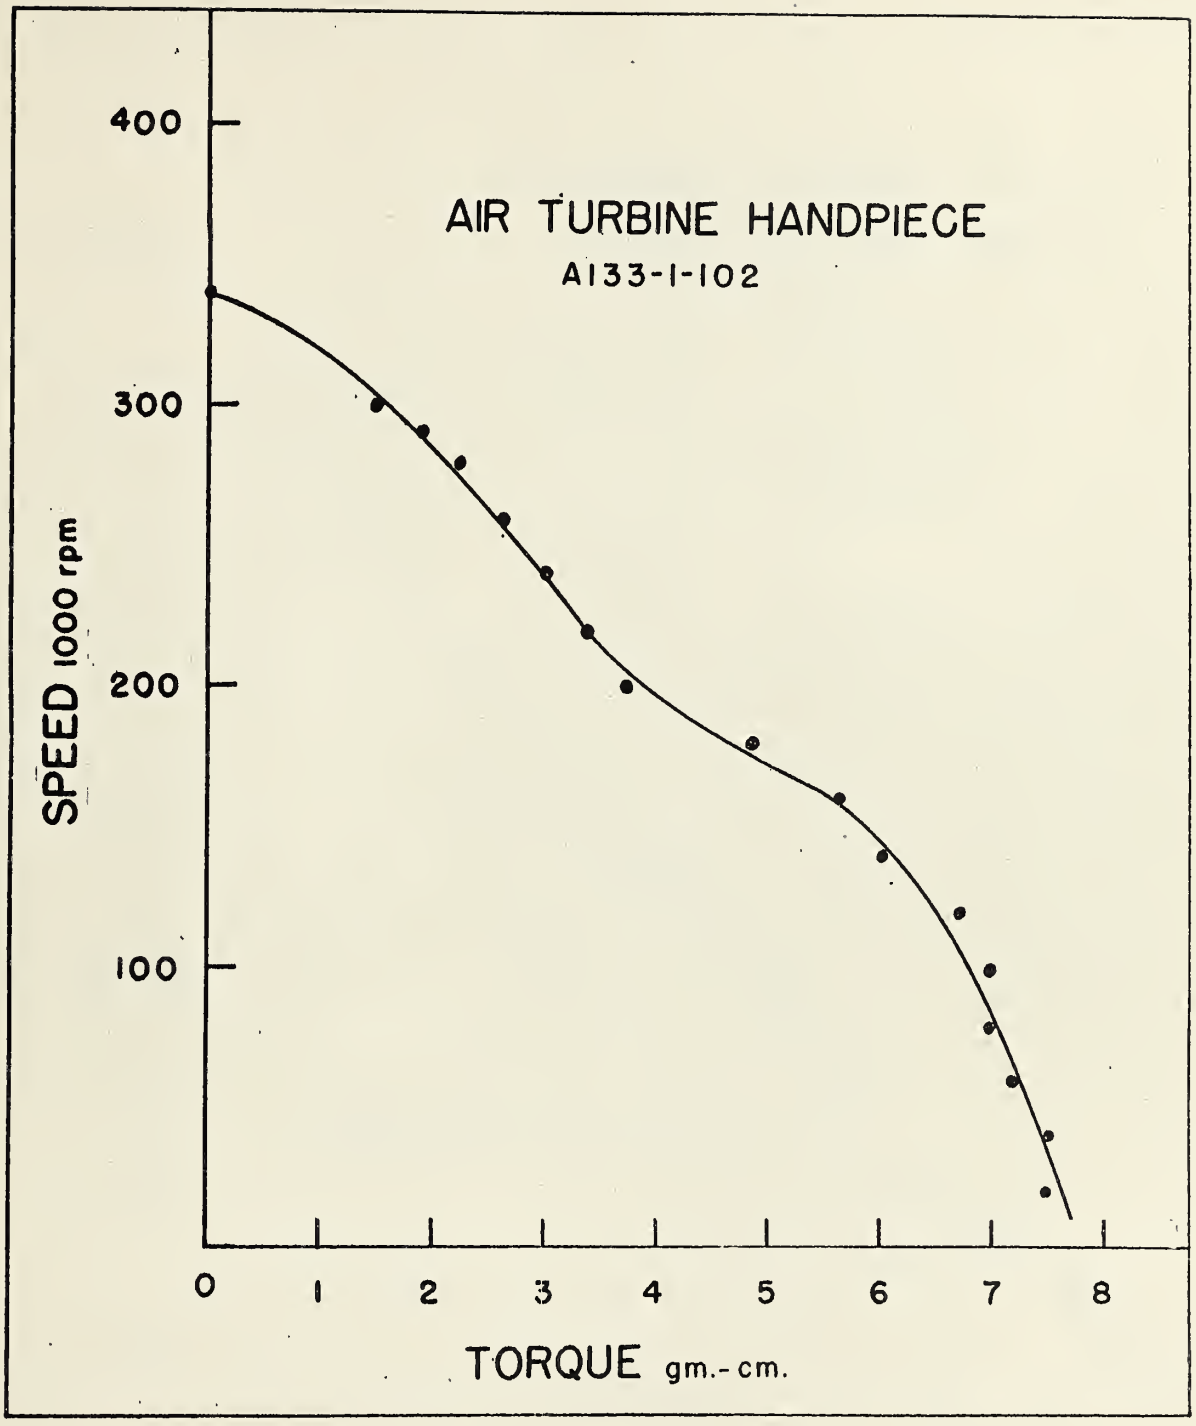


**Figure 7.** View showing the effect of grinding for dynamic balancing upon the shape of magnet cylinders.

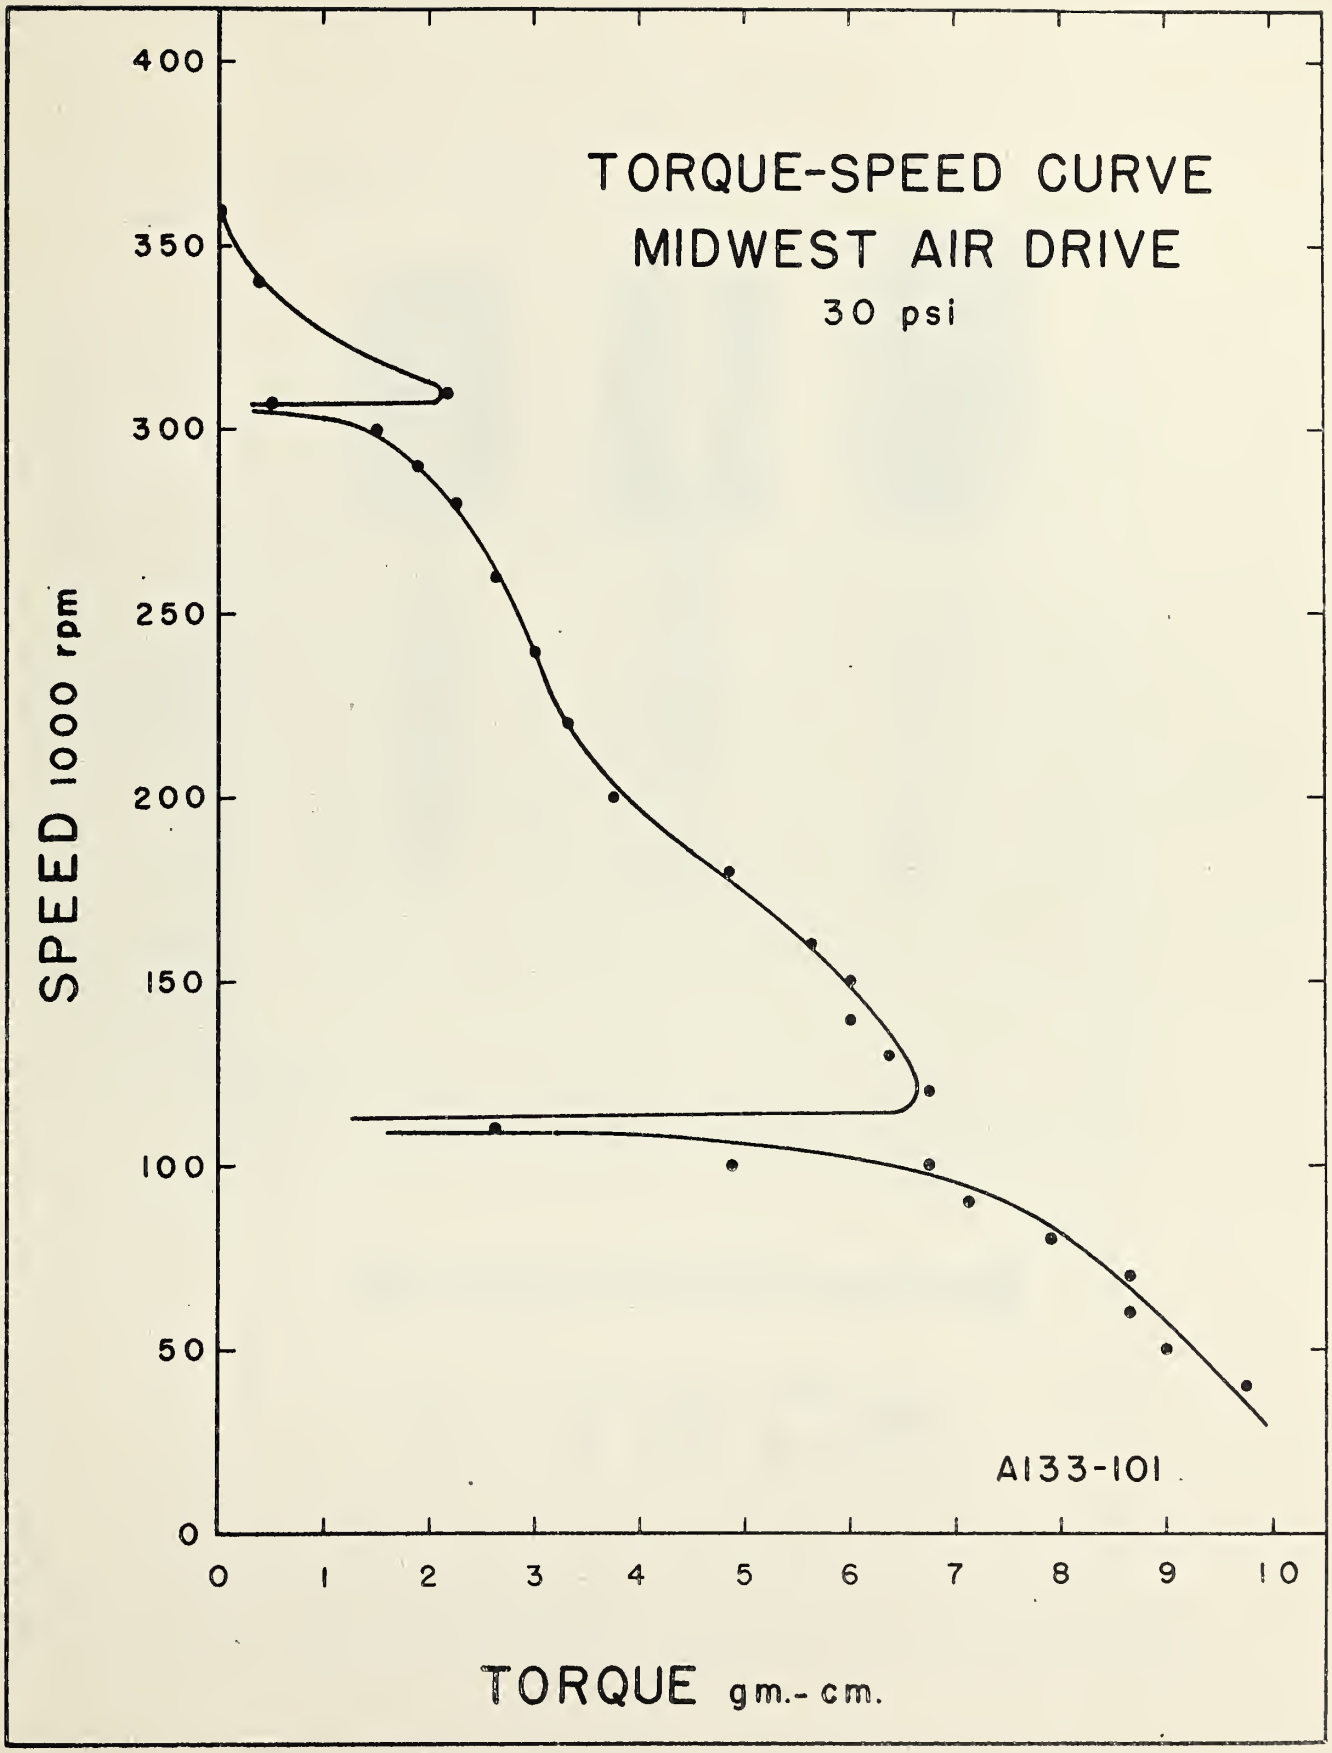


Figure 8. Torque - speed curves for various air turbine handpieces at 30 psi air pressure.

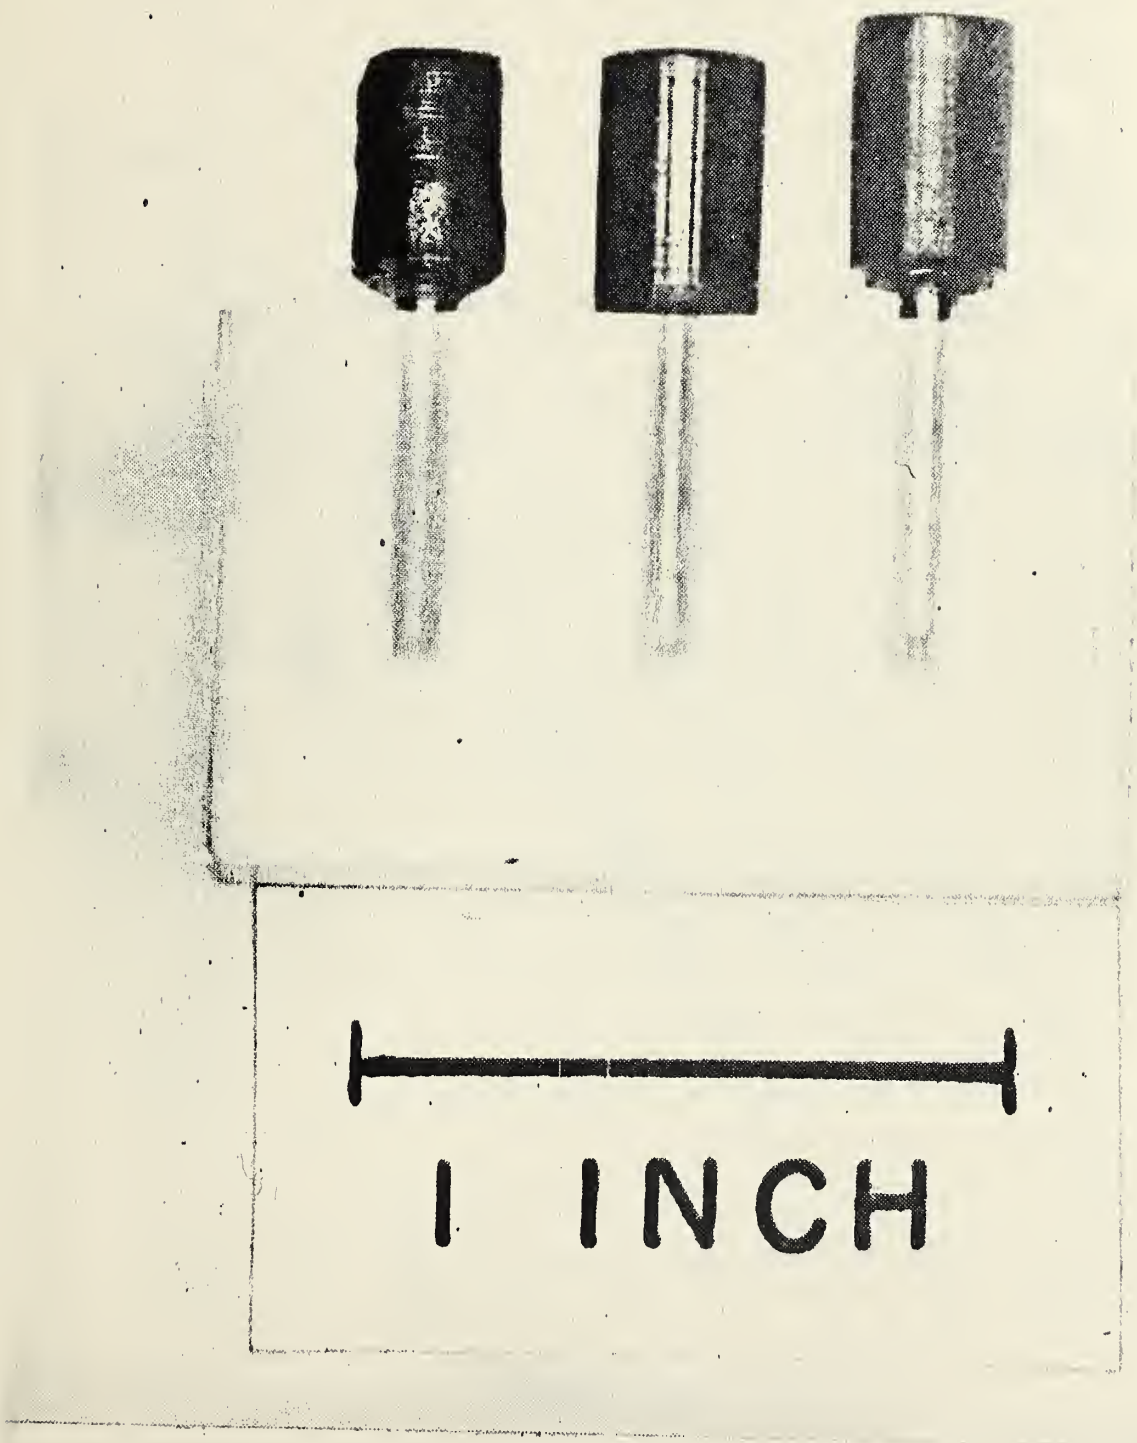


Figure 9. Power - speed curves for various air turbine handpieces, derived from the data of Figure 8.

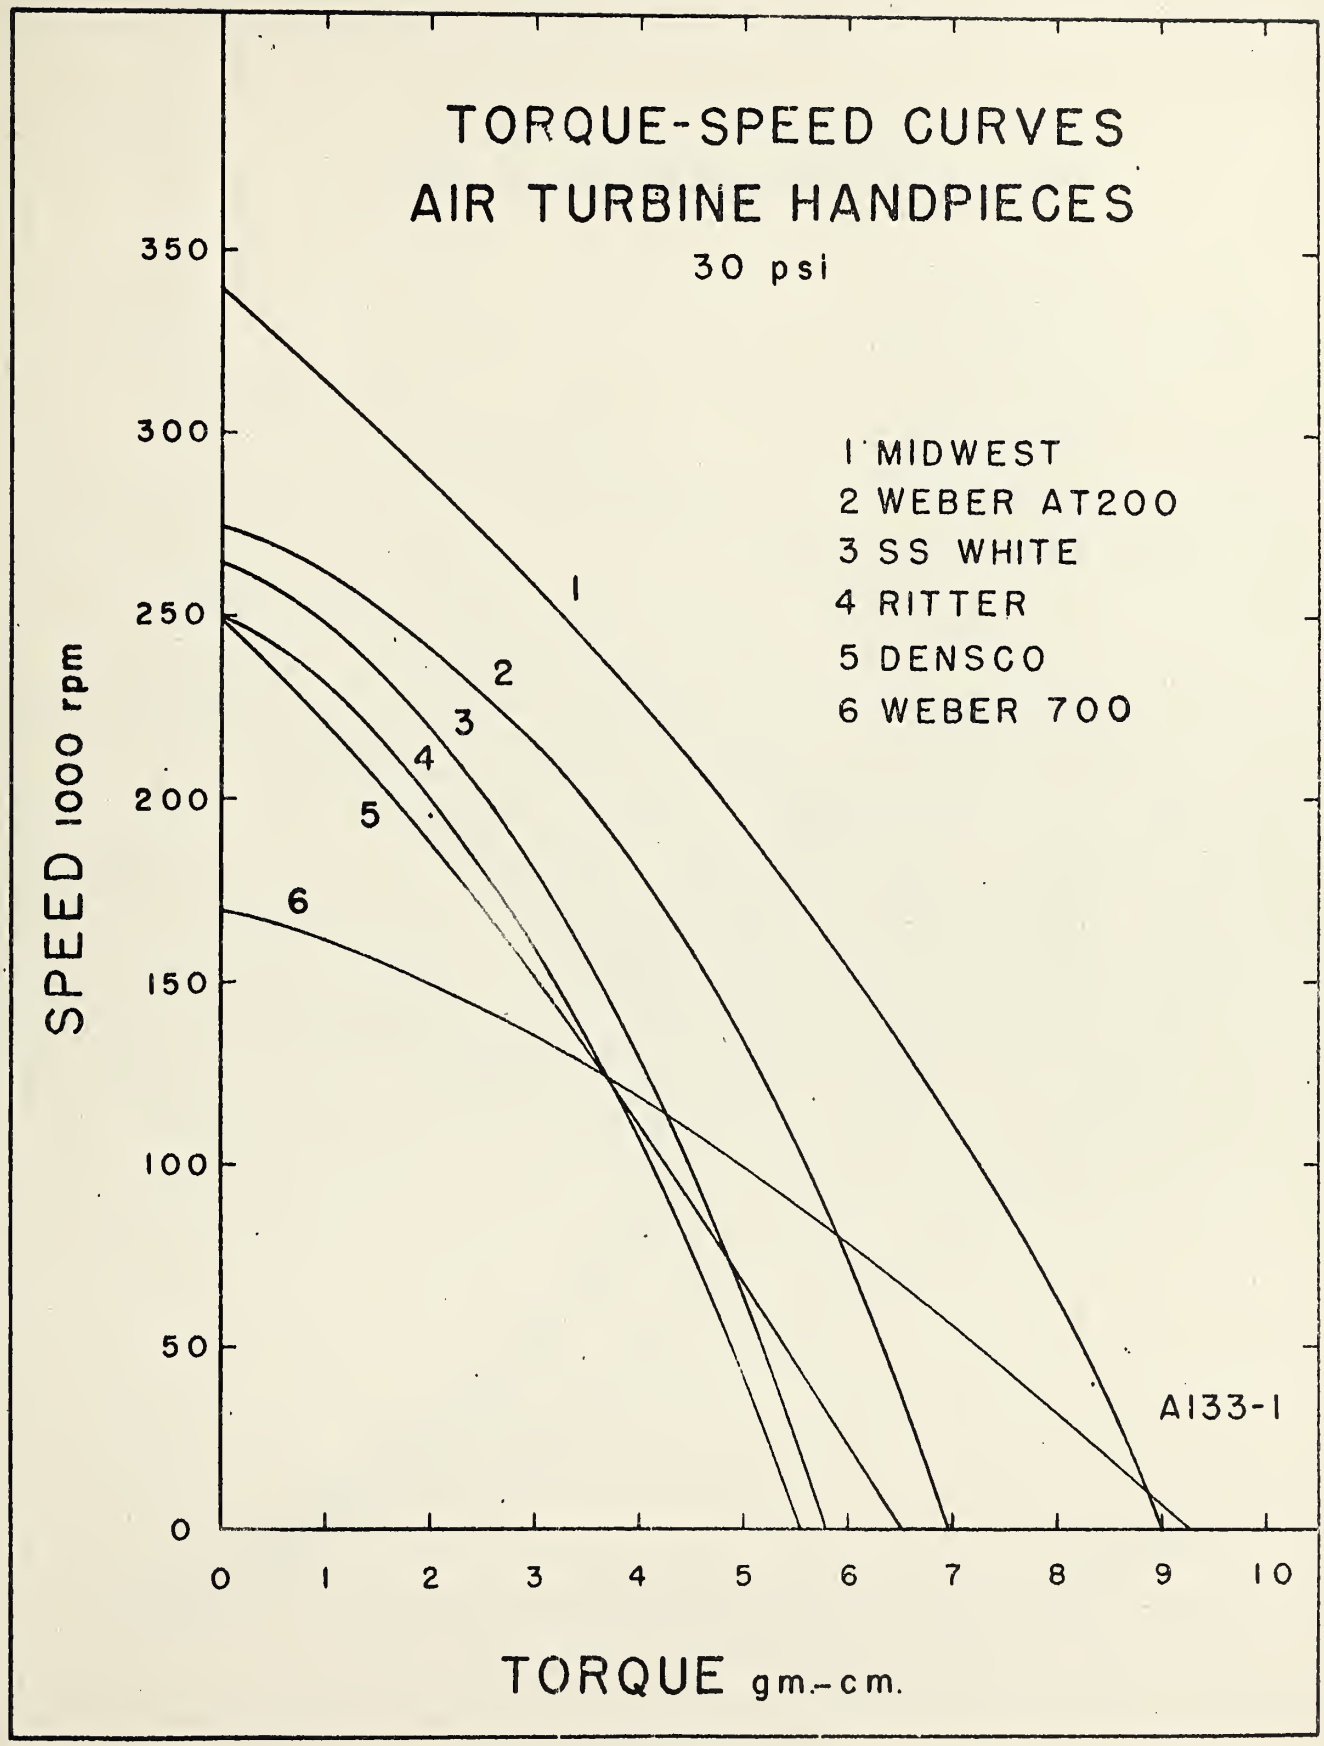


Figure 10. Torque - speed curves showing the effect of variation in air pressure.

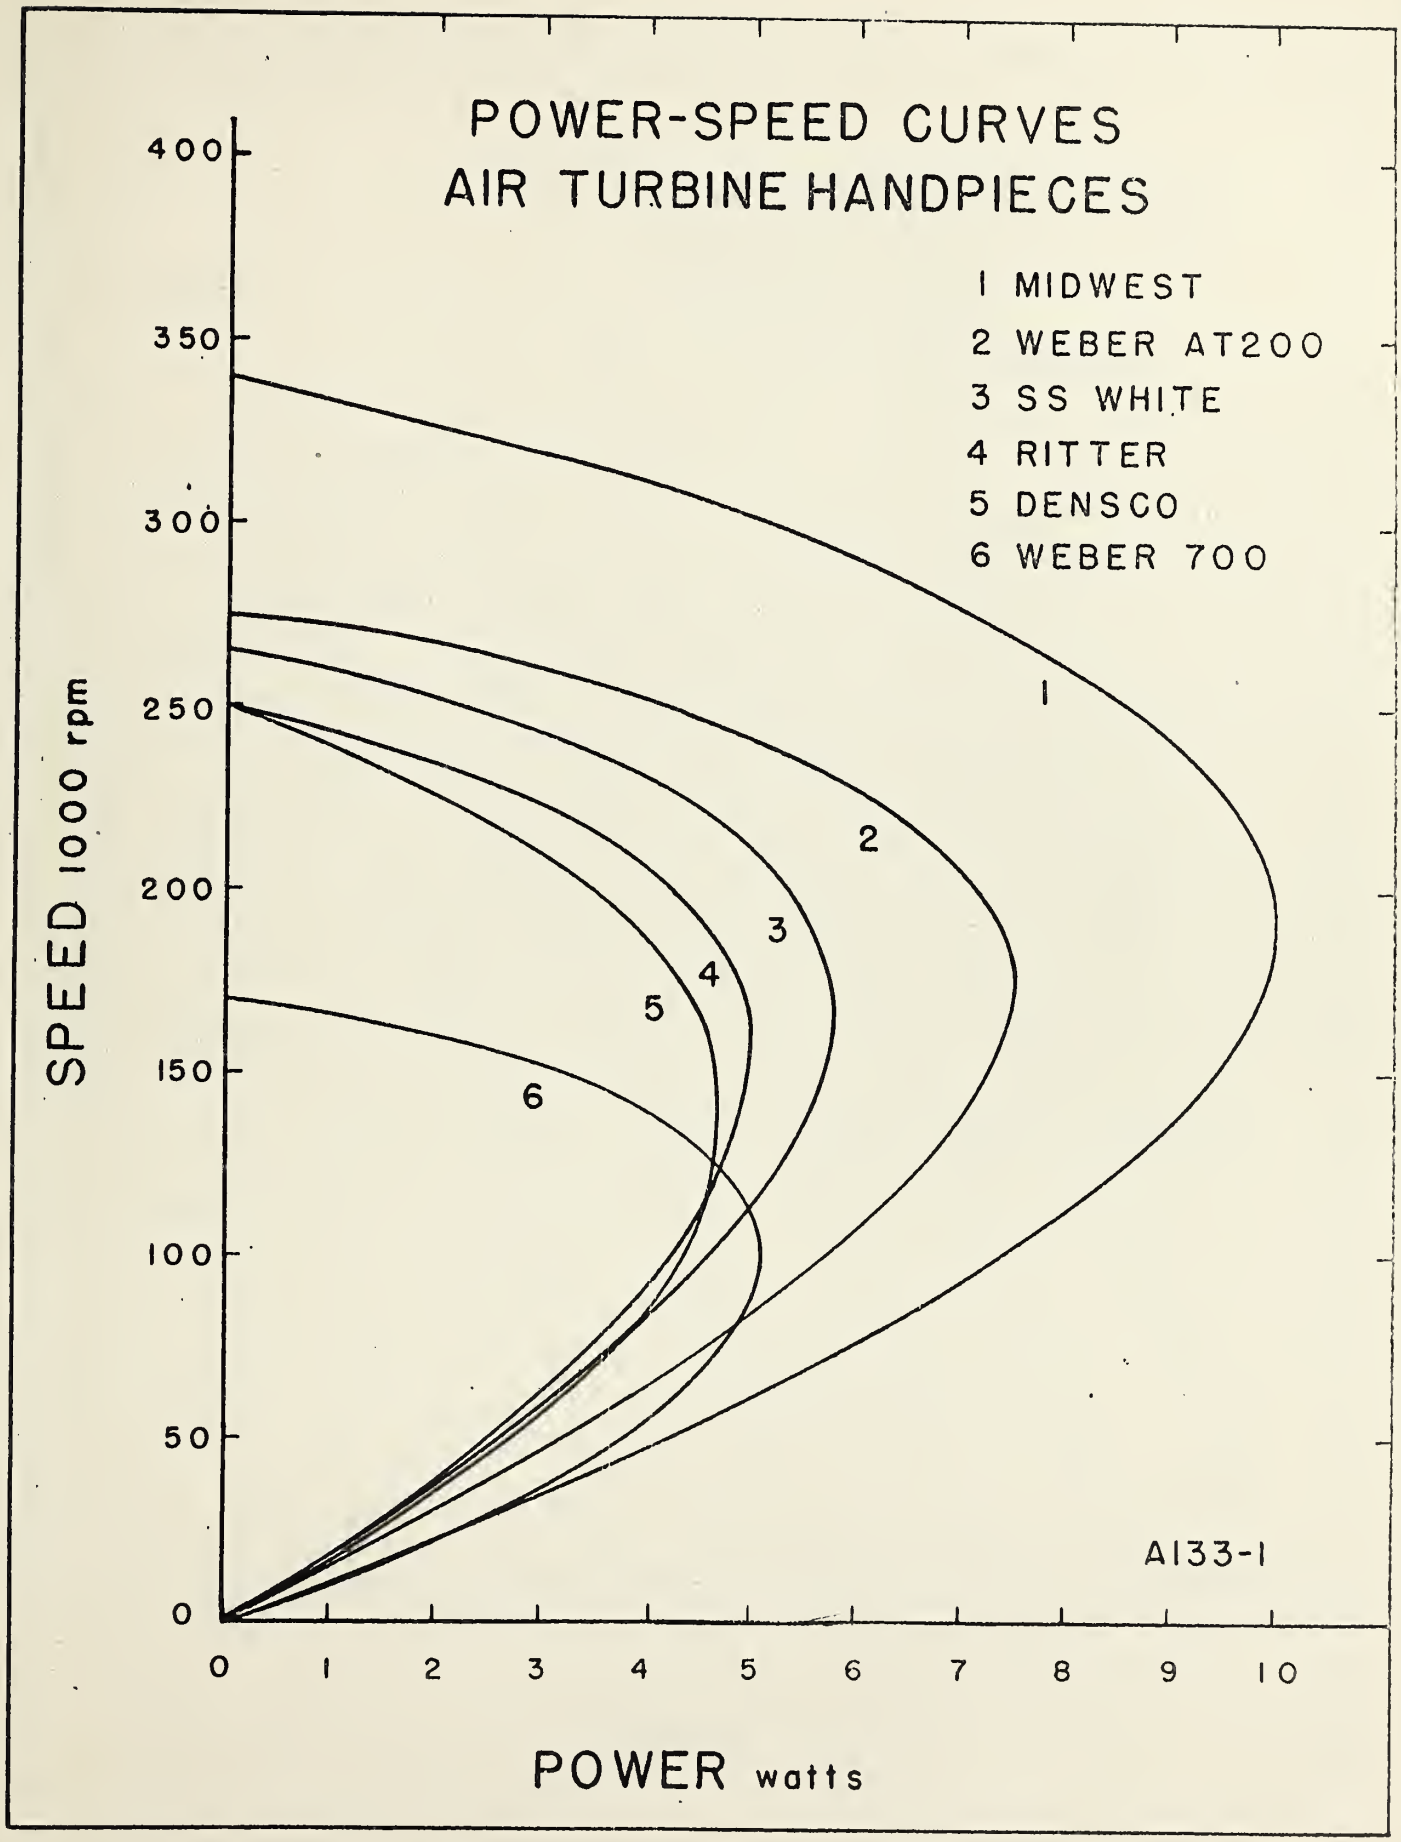


Figure 11. Power - speed curves showing the effect of variation in air pressure.

U. S. DEPARTMENT OF COMMERCE
Lewis L. Strauss, *Secretary*

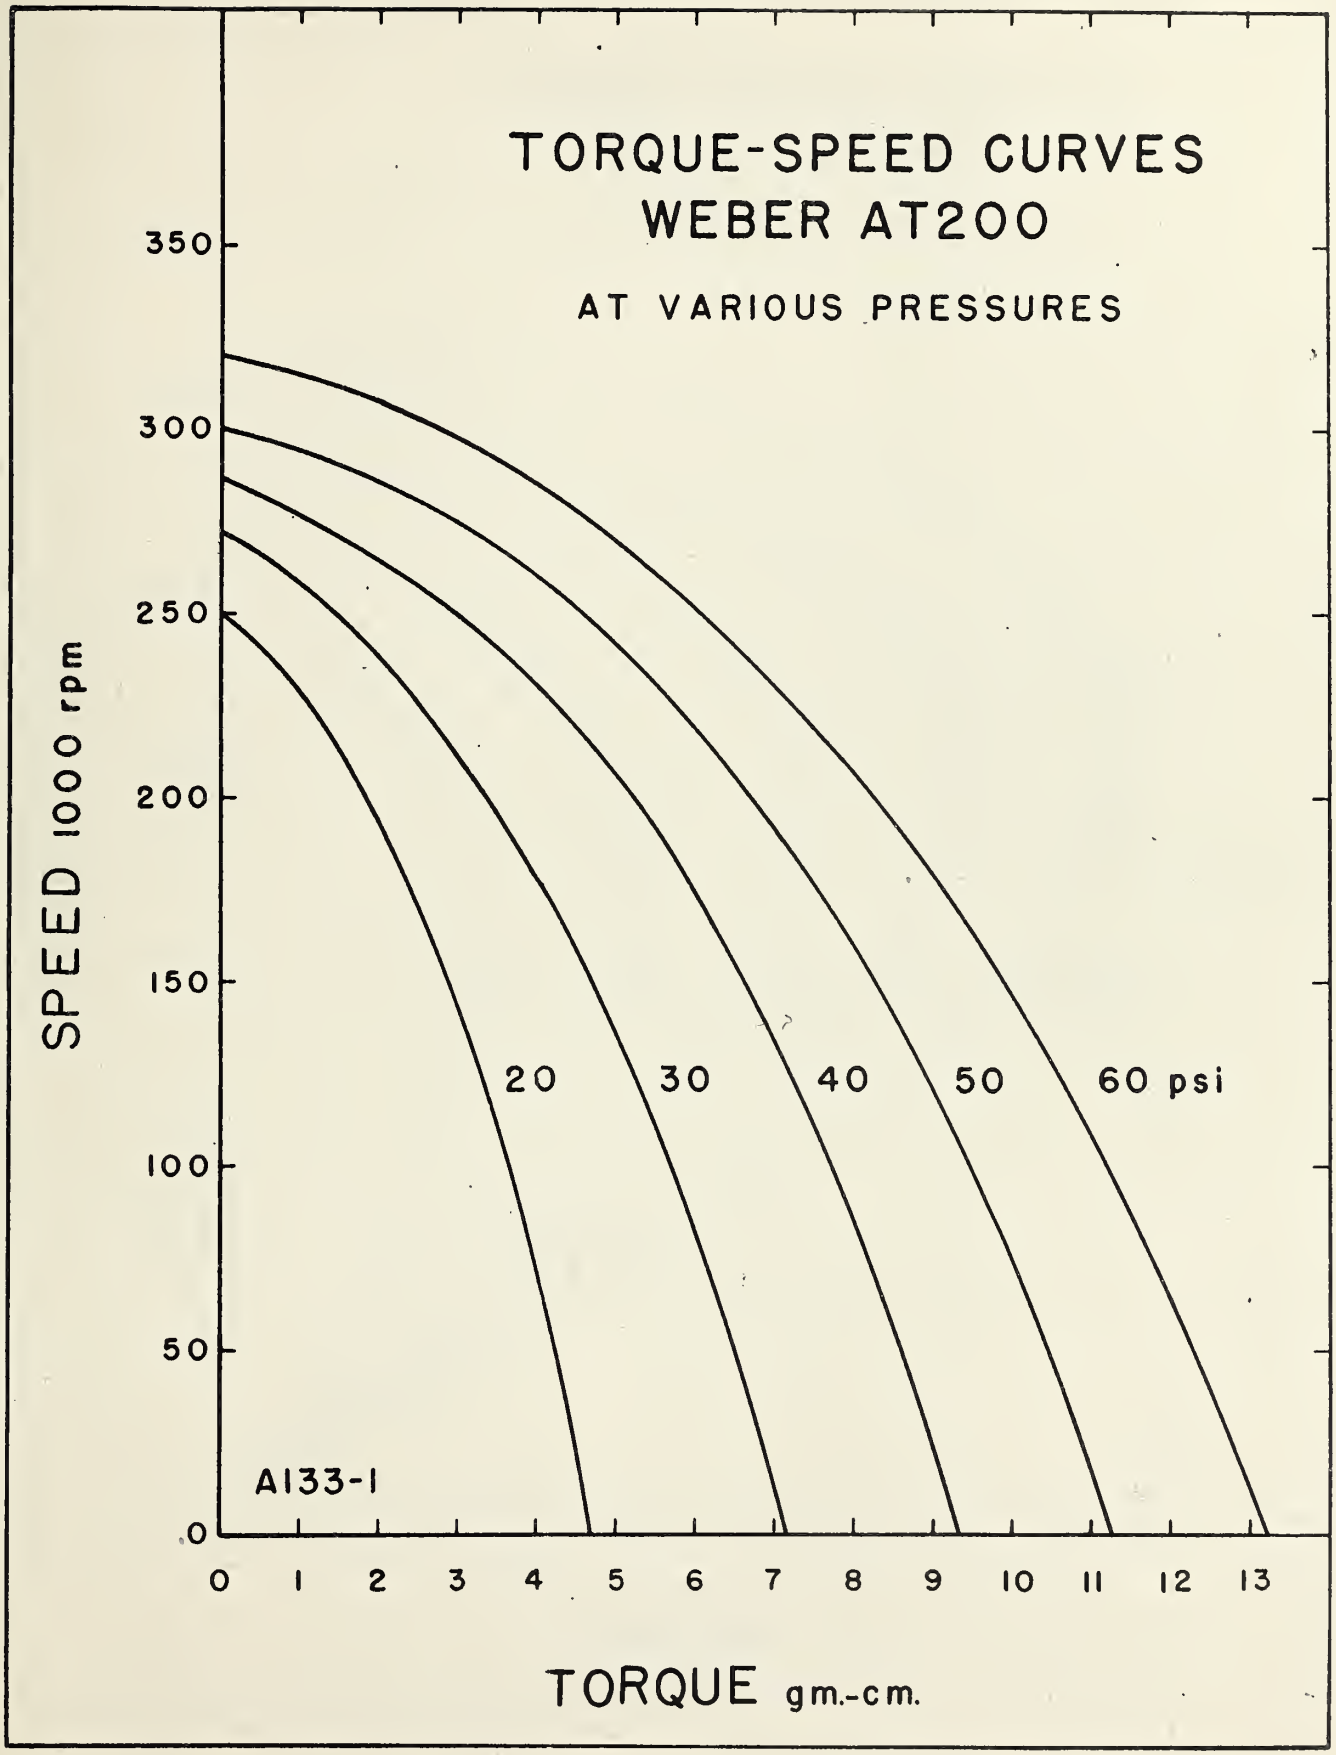NATIONAL BUREAU OF STANDARDS
A. V. Astin, *Director*

# THE NATIONAL BUREAU OF STANDARDS

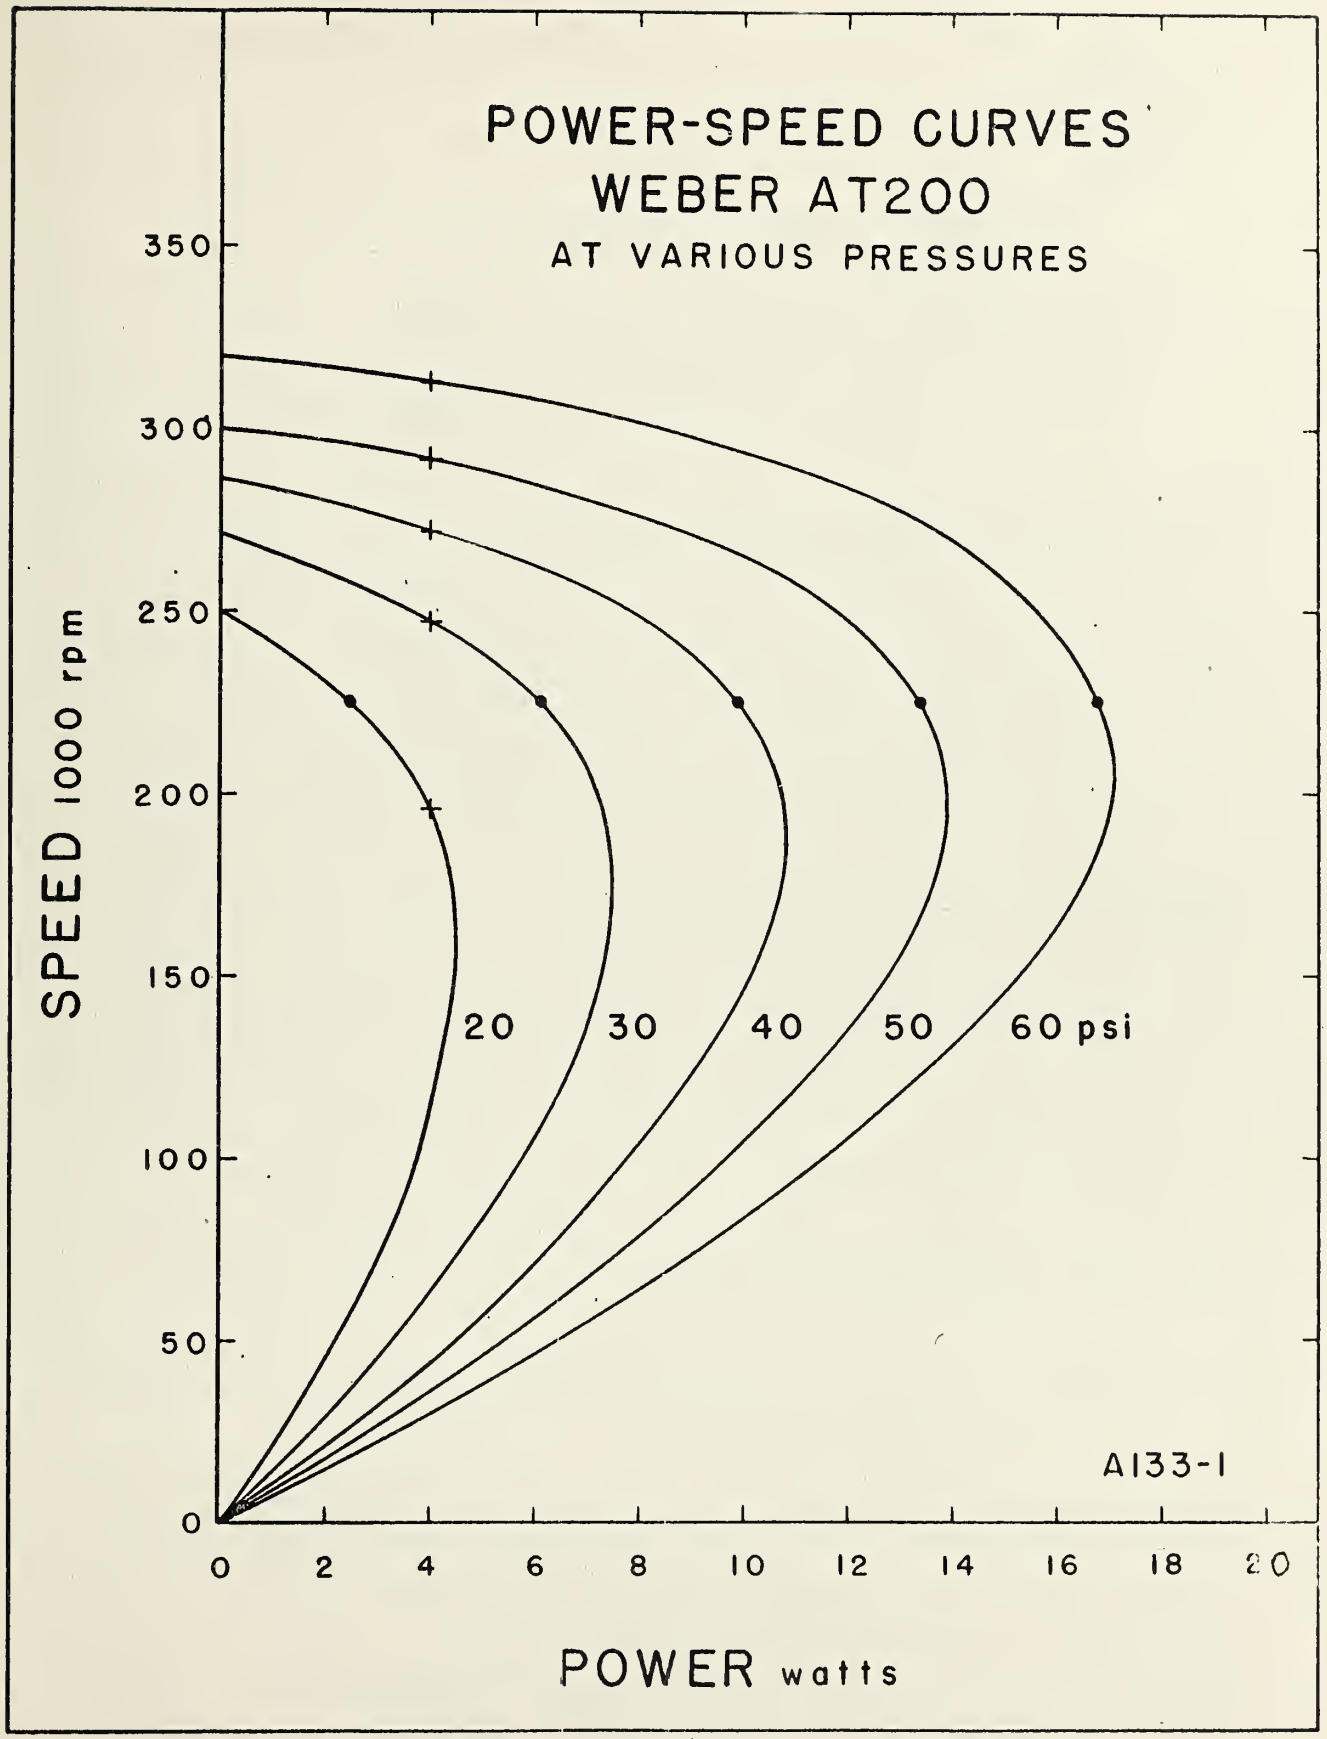The scope of activities of the National Bureau of Standards at its headquarters in Washington, D. C., and its major laboratories in Boulder, Colo., is suggested in the following listing of the divisions and sections engaged in technical work. In general, each section carries out specialized research, development, and engineering in the field indicated by its title. A brief description of the activities, and of the resultant publications, appears on the inside front cover.

## WASHINGTON, D. C.

**Electricity and Electronics.** Resistance and Reactance. Electron Devices. Electrical Instruments. Magnetic Measurements. Dielectrics. Engineering Electronics. Electronic Instrumentation. Electrochemistry.

**Optics and Metrology.** Photometry and Colorimetry. Optical Instruments. Photographic Technology. Length. Engineering Metrology.

**Heat.** Temperature Physics. Thermodynamics. Cryogenic Physics. Rheology. Engine Fuels. Free Radicals Research.

**Atomic and Radiation Physics.** Spectroscopy. Radiometry. Mass Spectrometry. Solid State Physics. Electron Physics. Atomic Physics. Neutron Physics. Radiation Theory. Radioactivity. X-rays. High Energy Radiation. Nucleonic Instrumentation. Radiological Equipment.

**Chemistry.** Organic Coatings. Surface Chemistry. Organic Chemistry. Analytical Chemistry. Inorganic Chemistry. Electrodeposition. Molecular Structure and Properties of Gases. Physical Chemistry. Thermochemistry. Spectrochemistry. Pure Substances.

**Mechanics.** Sound. Mechanical Instruments. Fluid Mechanics. Engineering Mechanics. Mass and Scale. Capacity, Density, and Fluid Meters. Combustion Controls.

**Organic and Fibrous Materials.** Rubber. Textiles. Paper. Leather. Testing and Specifications. Polymer Structure. Plastics. Dental Research.

**Metallurgy.** Thermal Metallurgy. Chemical Metallurgy. Mechanical Metallurgy. Corrosion. Metal Physics.

**Mineral Products.** Engineering Ceramics. Glass. Refractories. Enameled Metals. Concreting Materials. Constitution and Microstructure.

**Building Technology.** Structural Engineering. Fire Protection. Air Conditioning, Heating, and Refrigeration. Floor, Roof, and Wall Coverings. Codes and Safety Standards. Heat Transfer.

**Applied Mathematics.** Numerical Analysis. Computation. Statistical Engineering. Mathematical Physics.

**Data Processing Systems.** SEAC Engineering Group. Components and Techniques. Digital Circuitry. Digital Systems. Analog Systems. Application Engineering.

• Office of Basic Instrumentation.

• Office of Weights and Measures.

## BOULDER, COLORADO

**Cryogenic Engineering.** Cryogenic Equipment. Cryogenic Processes. Properties of Materials. Gas Liquefaction.

**Radio Propagation Physics.** Upper Atmosphere Research. Ionospheric Research. Regular Propagation Services. Sun-Earth Relationships. VHF Research. Ionospheric Communication Systems.

**Radio Propagation Engineering.** Data Reduction Instrumentation. Modulation Systems. Navigation Systems. Radio Noise. Tropospheric Measurements. Tropospheric Analysis. Radio Systems Application Engineering. Radio-Meteorology.

**Radio Standards.** High Frequency Electrical Standards. Radio Broadcast Service. High Frequency Impedance Standards. Electronic Calibration Center. Microwave Physics. Microwave Circuit Standards.

NBS